



## GUIDE

# Model-915-Series

Isotech

Distributed by AKRIBIS



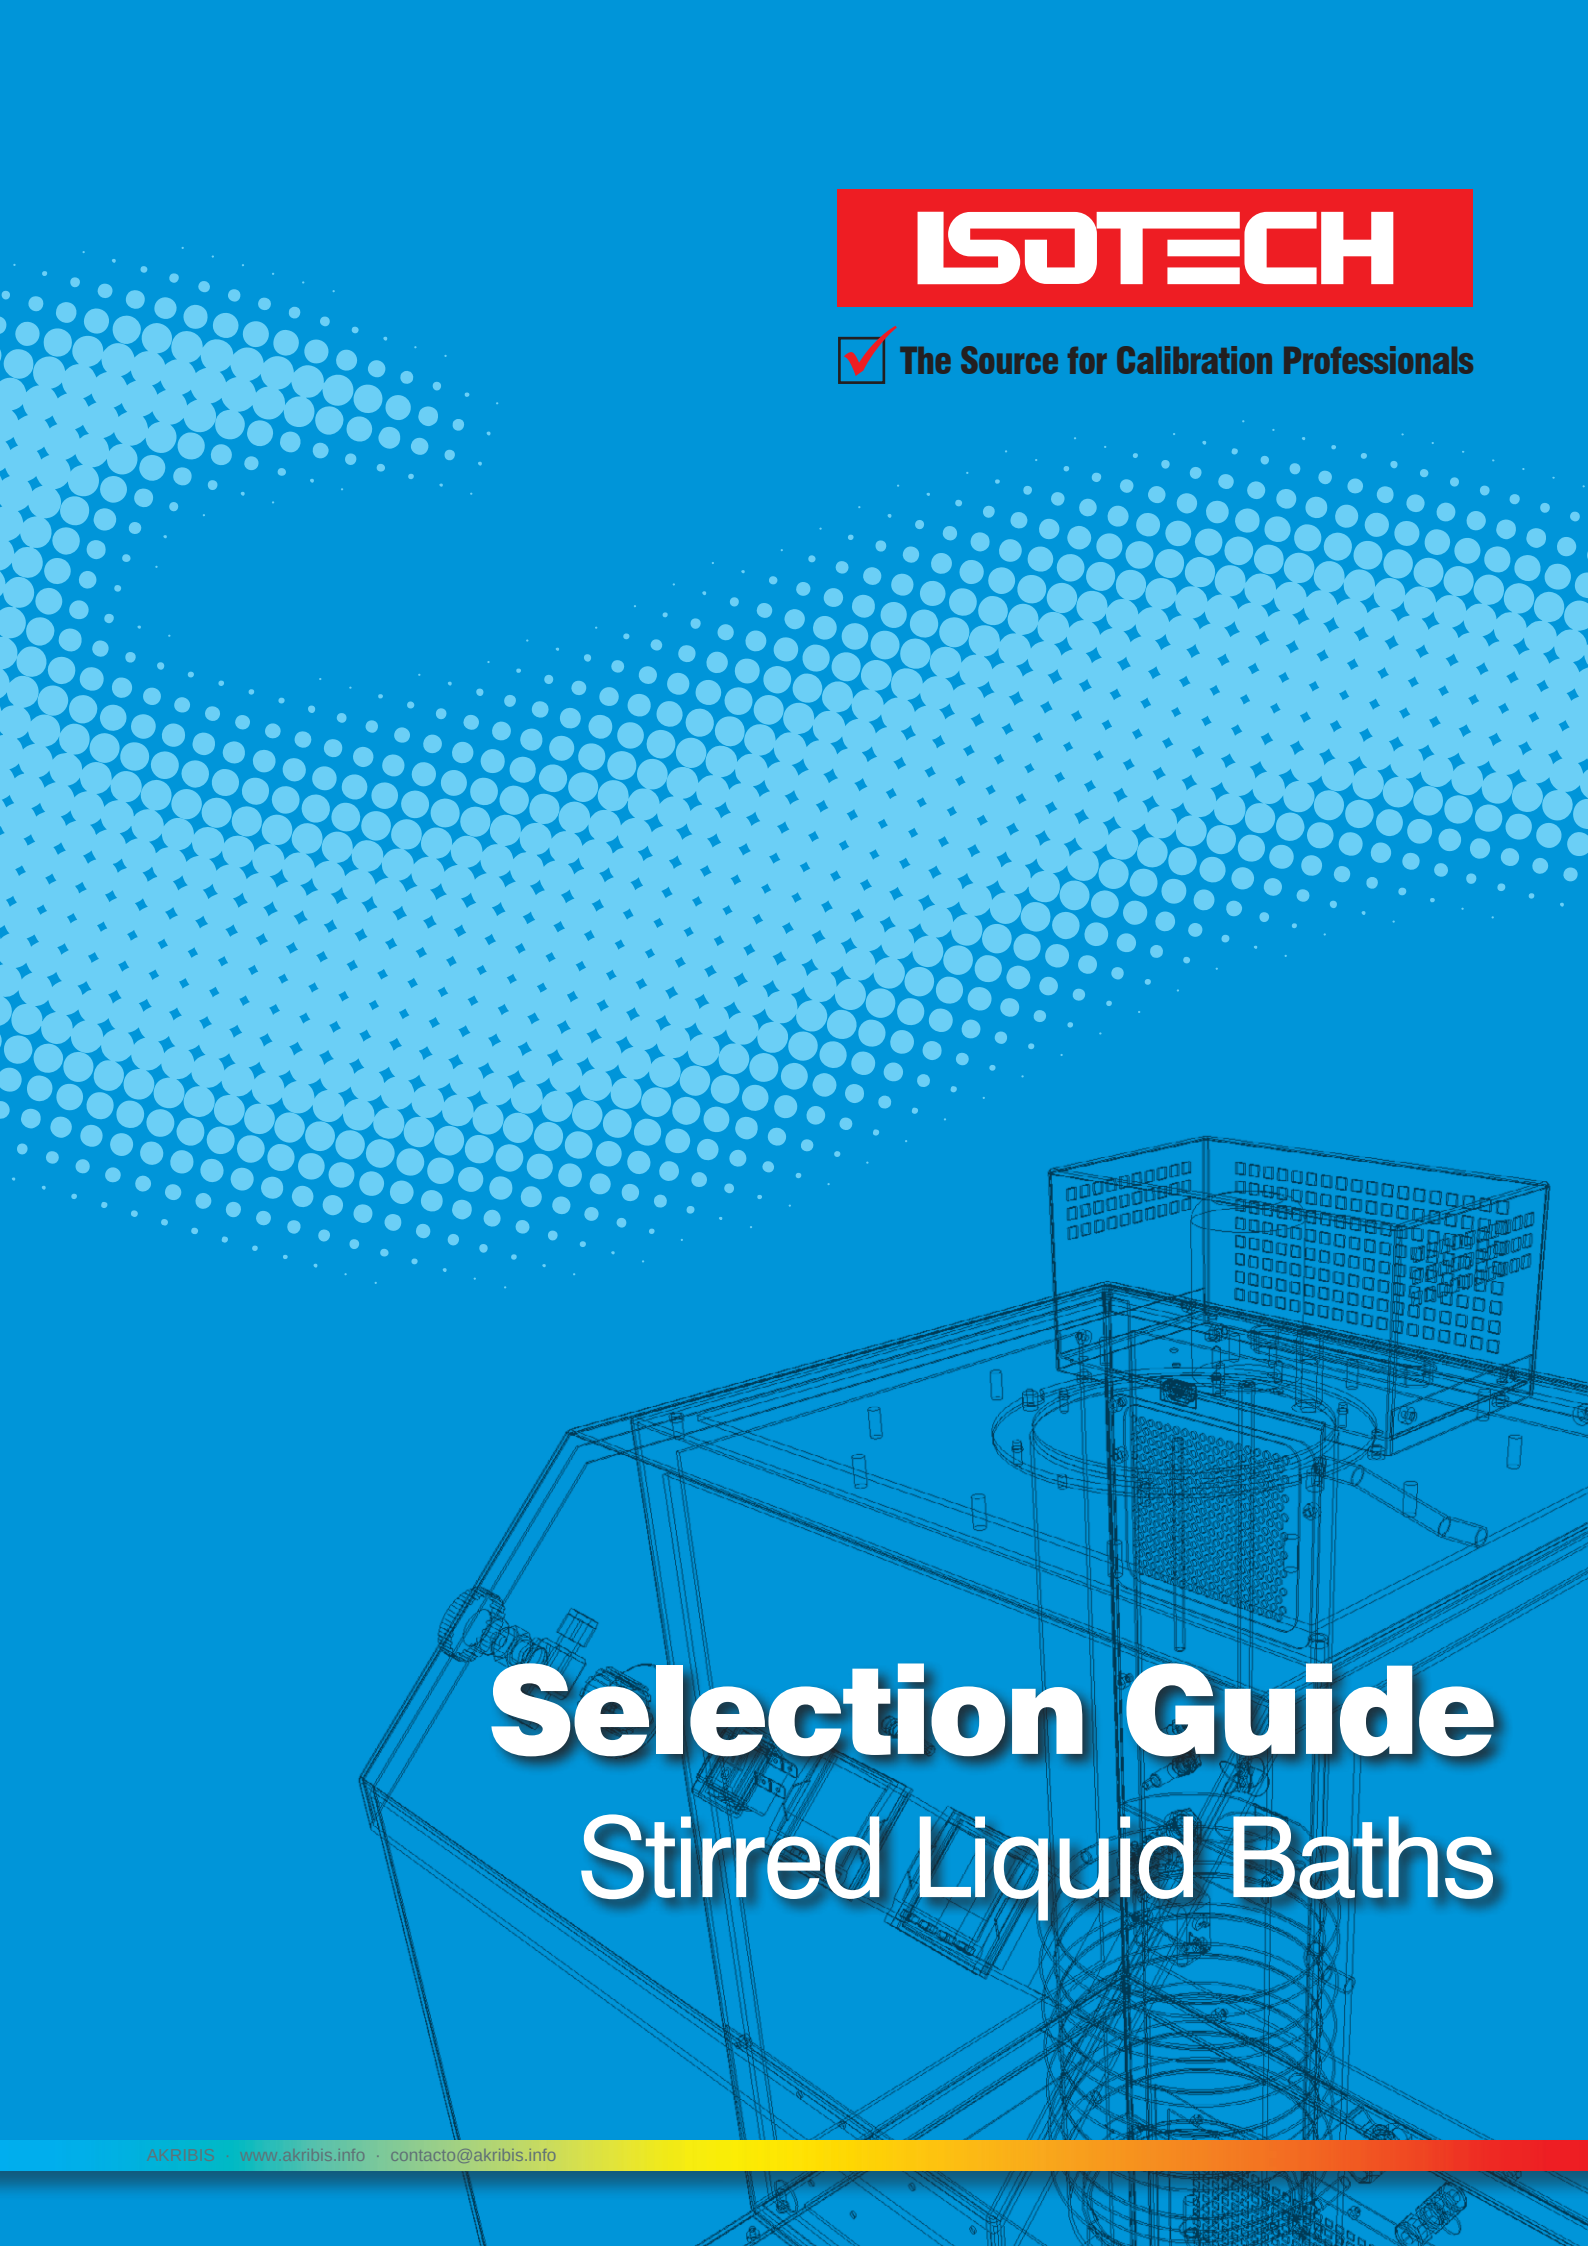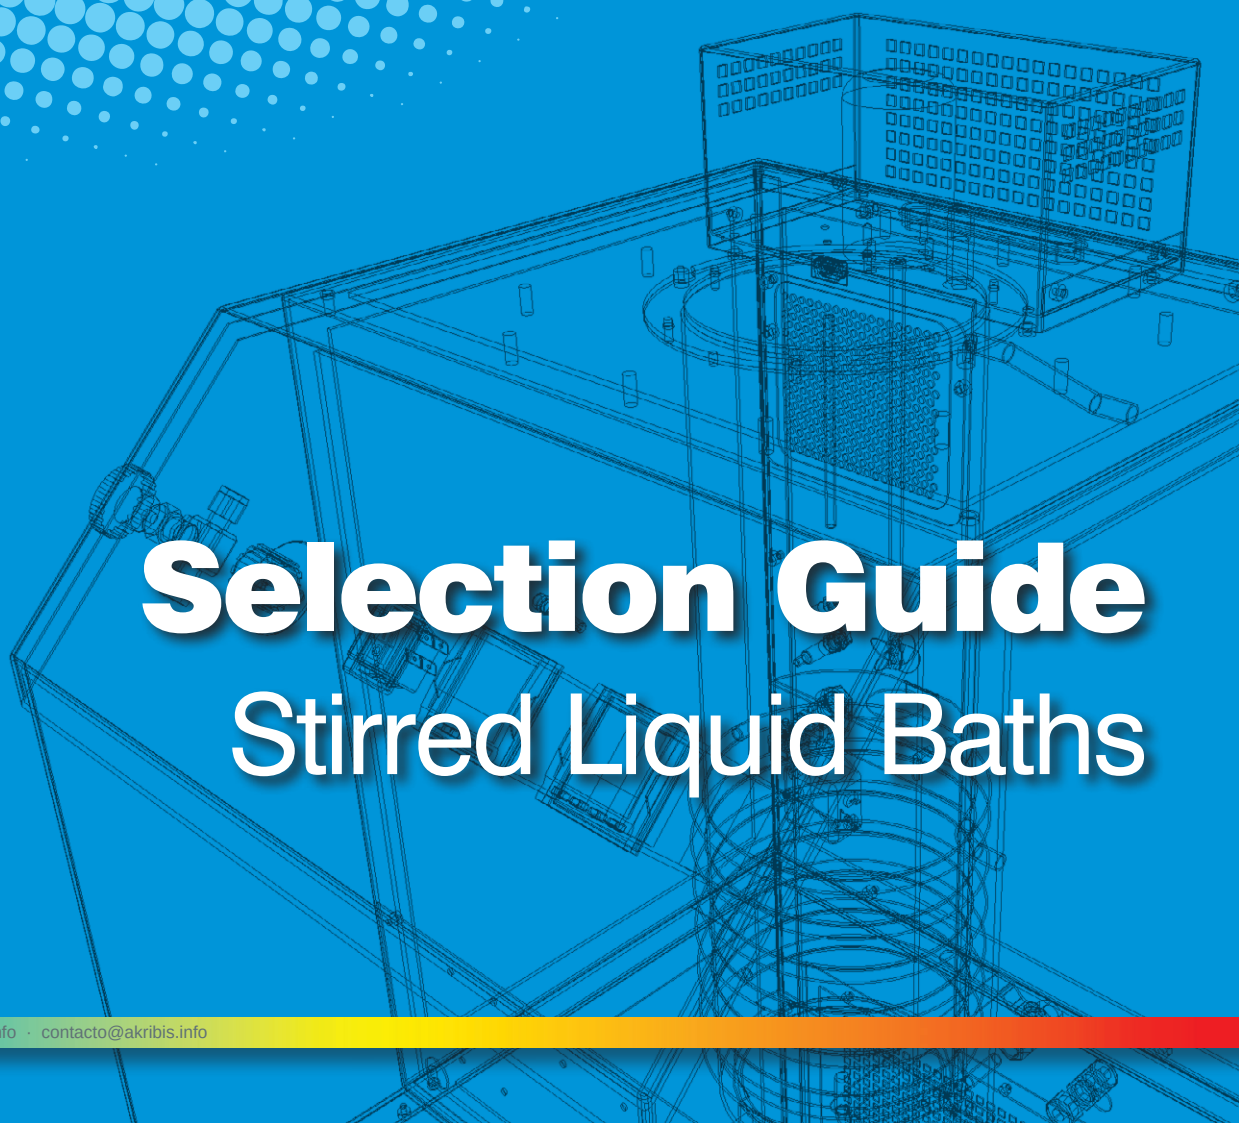

**ISOTECH**



**The Source for Calibration Professionals**

# **Selection Guide**

## **Stirred Liquid Baths**

# How to Select a Stirred Liquid Bath

**Use this guide to avoid make costly mistakes when selecting stirred liquid baths**

## One: Depth

Depth matters, the "Supplementary Information for the ITS-90" published by BIPM advises that for metal sheath thermometers, "Immerse the thermometer from 15 to 20cm between -50°C and 50°C and from 20 to 27cm at 200°C and above" (BIPM,p.93, 1990).

*Ensure you select a bath that can offer suitable immersion for low uncertainty calibration of platinum resistance thermometers*

Isotech laboratory baths offer immersion from 300mm with adequate depth to avoid significant stem conduction / immersion error.

## Two: Homogeneity


With comparison calibration a thermometer with known characteristics is compared to the thermometer we want to calibrate, relying on the "Zeroth Law of Thermodynamics".

If the temperature in the bath is not homogenous (uniform) there will be differences in temperature between the thermometers.

Isotech laboratory baths use sophisticated designs to avoid poor temperature distribution from simple square tanks.


Advanced parallel tube designs allow the heating and cooling to take place in a chamber separate from the calibration volume. The geometry and flow ensure the best uniformity and lowest calibration uncertainties.

In addition to the best design to ensure the best homogeneity we use sophisticated temperature control techniques. As well as PID control we use power feedback to stabilise against supply voltage variation and advanced digital filtering ensures high integrity of measurement correcting for drift and rejecting noise.


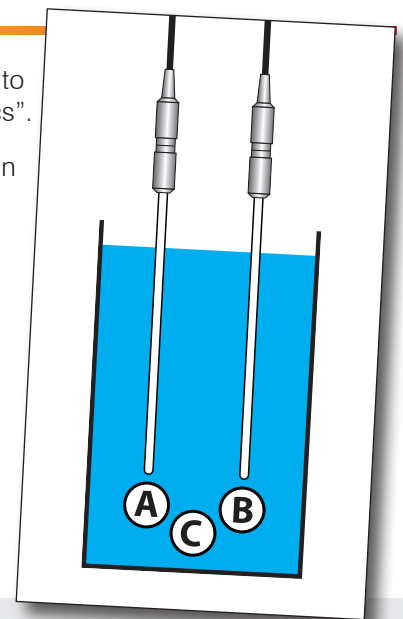


## Three: Cost of Ownership

Stirred liquid baths most commonly use suitable oils to higher temperatures and alcohol or specialist fluids for low temperatures. These fluids can be costly and will require replacing from time to time. This is of course true for all stirred liquid calibration baths and the cost of both the initial and on-going requirement needs to be considered when selecting a bath.

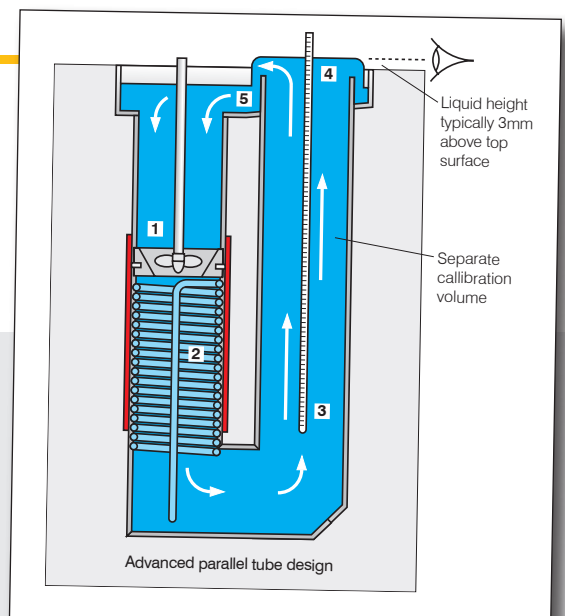

Isotech baths are purpose designed for thermometer calibration with cylindrical calibration volumes of good depth. Compared to other large rectangular designs Isotech baths require less fluid for the same depth and can offer significant initial and on-going cost savings.

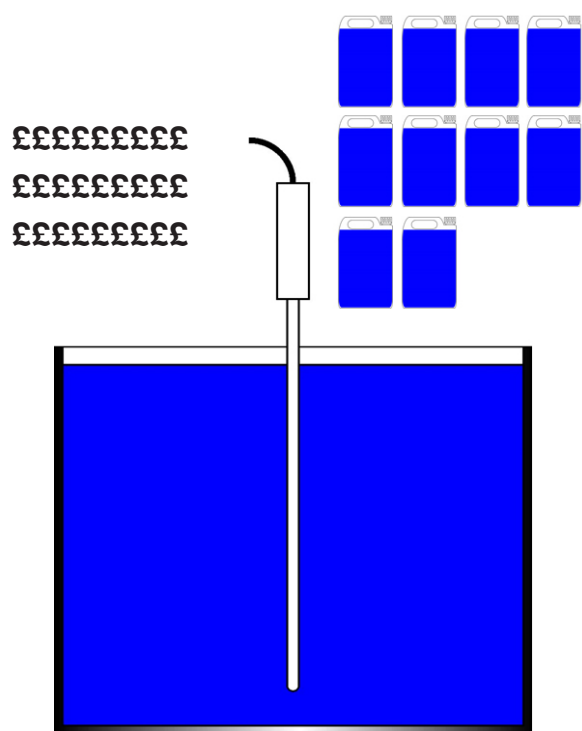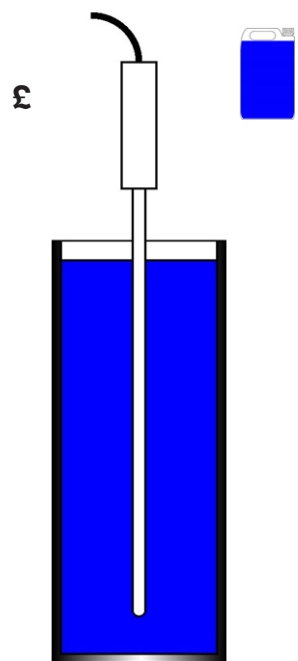

# Recommendations

Use a true thermometry bridge to compare the thermometer under test to the standard thermometer. This method gives the smallest uncertainties. Isotech can provide further advice and training. We have over 30 year's experience and operate a UKAS (ISO 17025) Laboratory.

Using our baths our CMC using stirred liquid baths is from 4 to 7mK, our full schedule is on the website.



| Measured Quantity<br>Instrument or Gauge | Range                                                                           | Calibration and Measurement<br>Capability (CMC) Expressed<br>as an Expanded Uncertainty<br>( <i>k</i> = 2) | Remarks |
|------------------------------------------|---------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------|---------|
| TEMPERATURE (cont'd)                     |                                                                                 |                                                                                                            |         |
| Platinum resistance<br>thermometers      |                                                                                 |                                                                                                            |         |
| Calibration by comparisons               | - 80 °C to - 40 °C<br>- 40 °C to + 50 °C<br>50 °C to 156 °C<br>156 °C to 300 °C | 7.0 mK<br>4.0 mK<br>5.0 mK<br>6.5 mK                                                                       |         |

Extract from UKAS Schedule

# Isotech Laboratory Bath Selection Guide

## Parallel Tube Liquid Bath - **Model 915**



- Best performance
- -65°C to 300°C
- Removable Chiller Probe

*25 Years of  
proven use*

## Parallel Tube Liquid Bath - **Model 785**



- Best performance
- -80°C to 300°C.
- Integral Cooling
- 485mm Immersion

*Updated 915  
– recommended  
for new  
installations*

## Stirred Liquid Bath - **Model 796**



- Good Value
- -80°C to 300°C
- 470mm Immersion

*Competitively  
Priced  
Laboratory Bath  
with extended  
immersion*

## Stirred Liquid Bath - **Model 798**



- -80°C to 300°C
- Good Value
- 300mm Immersion

*Competitively  
Priced  
Laboratory Bath  
with standard  
immersion*

For more information and full specifications: [www.isotech.co.uk](http://www.isotech.co.uk)



✓ The Source for Calibration Professionals

Telephone: +44 (0)1704 543830

Fax: +44 (0)1704 544799 Email: [info@isotech.co.uk](mailto:info@isotech.co.uk) Web: [www.isotech.co.uk](http://www.isotech.co.uk)  
AKRIBIS • [www.akribis.info](http://www.akribis.info) • [contacto@akribis.info](mailto:contacto@akribis.info)  
**Isothermal Technology Limited** Pine Grove, Southport, Merseyside PR9 9AG England

